Operation and Storage Environments

Operating Temperature: +5 ° C to +40 ° C

Operating humidity: 20% RH to 80% RH

Operating pressure: 86kPa to 106kPa

Storage temperature: -10 ° C to +55 ° C

Storage pressure: 50kPa to 106kPa

Storage humidity: ≤93%RH

Product warranty

LED dental lamp warrantly period of 12 months.

Packing list

LED lamp x 1 | Handle shell x 2 | Decoration cover x 1 | Hexagonal wrench x 1

Standard symbols


Attention



Cataloguenumber


Keep dry


Refer to instruction manual/booklet


WEEE



EuropeanUnion agent


For indoor use only


Fragile



CE marked product


Vertical up


Manufacturer



LOT Number



COXO®



Foshan COXO Medical Instrument Co.,Ltd.
No. 17, Guangming Ave., New Light Source Industrial Base, Nanhai
National High-tech Zone, Foshan 528226, Guangdong P.R. China

EU REP **Lotus NL B.V.**
Koningin Julianaplein 10, 1e Verd, 2595AA, The Hague, Netherlands.
E-mail: info@lotusnl.com Tel: +31644168999

Ver:1.7 Revision Date:20251101 AE1295

USERS GUIDE

⚠ WARNING

- The function of the dental light is to illuminate the oral cavity of the patient during dental operations.
- The dental light must be used by qualified staff.
- Installation of the system must only be performed by specialized staff.
- Check that the power voltage, shown on the data plate, corresponds to the mains voltage.
- Do not block the dental light beam for patients at risk (i.e. with eye conditions). Use correct protection and precautions.
- The dental light must be installed on a specific control and supply device, such as a dental unit, or with an electrical system that complies with standard IEC 364-1 and “national regulations for installation of electrical systems in areas for medical use”.
- Do not carry out any maintenance work when the power is on; disconnect the power cable from the mains beforehand.
- Do not introduce items or tools into slits in the dental light head that could touch live points.
- Patients at risk (e.g. children with eye diseases) must not stare at the dental light beam.
- Always use appropriate protection devices and precautions. Manufacturer suggests using the protective eyeware BLUE-BAN or BABY BLUE-BAN (for children).
- Not suitable for installation in environments containing flammable gas.
- Do not spray detergents-disinfectants directly on the head.
- For cleaning plastic parts of the dental light, Do not use detergents disinfectantscontaining: AMMONIUM HYDRIXIDE –SODIUM HYDROXIDE – METHYLENE CHLORIDE – METHYL ALCOHOL. Failure to comply with this indication might cause: • risk of breakage of plastic parts.
- Do not carry out maintenance or replacement work on parts other than those shown in the manual. Any operation not indicated in the manual could compromise the safety aspect of the device.
- Disinfect surfaces with hydroalcoholic disinfectants.
- The dentist is obliged to used the disposal protection sleeves on the handles of the dental light or ensure that versions without this possibility are sterilized.


Technical data


1. Power voltage (without transformer): AC 12-24V,50/60Hz
2. Absorbed power: 15VA
3. Lux: ＞30000lux (distance spot 700mm)
4. Luminous spot dimensions: ＜180x90mm (distance spot 700mm)
5. Color temperature: 4000-6400K
6. Shaft dimensions: 0-90mm
7. Axis of rotation diameter:φ22mm
8. LED service life:5000H
9. Net Weight:1.6Kg

Intended Use

This product is intended to provide illumination for dentists during oral surgery or diagnosis.

Structure and composition

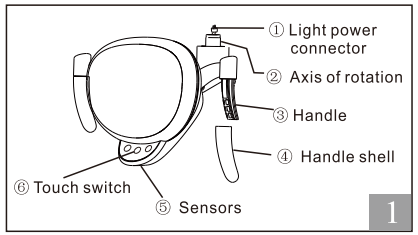

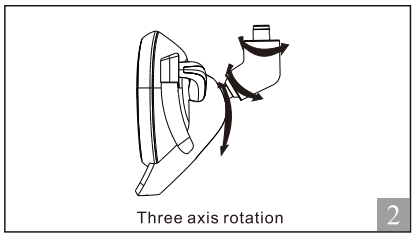



Installation

1. Handle mounting and dismounting:

As shown in Fig.3,

- Place handle shell④ into the handle③
- To remove the handle shell④,press the snap ⑪ and pull it out.





2. connection to the power supply connector:

As shown in Fig.4,

- Put ⑨ on ⑦;
- Connet ① and ⑩;
- Insert ② into ⑦ and fixed with ⑧.

Caution:

* Before installation,please confirm the power supply is AC12-24V, else will cause dental light damage.
* The dental light arm force must be over than 1.6Kg.

Instructions for use

This dental light has manual and sensor control modes.

1.Turning on and off

-Touch switch: touch the switch to turn on and off, as shown in Fig.5


-Sensors:move near to the sensor up to a maximum distance of 80mm,as shown in Fig.6


2.Adjustment of light intensity

-Touch switch: Continue to touch the right button to increase the light, continue to touch the left button to reduce the light,as shown in Fig.5, when it reaches the limited intensity,the machine will beep.

-Sensors:place the hand near the sensor until desired intensity is reached,from the maximum to the minimum level and from the maximum to the maximum level,as shown in Fig.5, when it reaches the limited intensity, the machine will beep.

- When the dental light is turned on, the intensity will be at the level memorized when it was turned off last time.

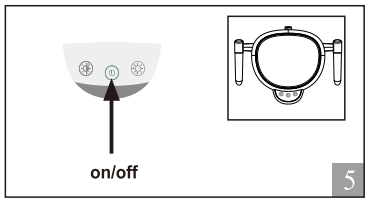

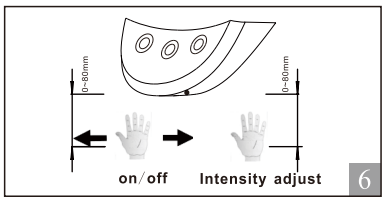

Cleaning and disinfection

1. For cleaning, manufacturer recommends using the detergent clean with a soft cloth and isopropyl alcohol.
2. The light handles should be cleaned before each use.
3. Hydroalcoholic disinfectants with 70% isopropyl or ethyl alcohol are suitable for disinfection.
4. For cleaning plastic parts , Do not use detergents-disinfectants containing ammonium Hydroxide - Sodium Hydroxide - Ethylene Chloride -Methyl alcohol.
5. Prohibited the use of corrosive chemicals cleaning.

Caution:

* Any parts of the lamp can not be sterilized.